

# << Develosil Column >>

## TEST REPORT


Packings	Develosil	ODS-HG, 5 $\mu$ m	Batch No.	1Y090919
Column size	Inner diameter	4.6 mm	Length	150 mm
End fitting type	NW			
Mfg. No.	12032065C-OI			

### Operating conditions

Mobile phase	: Acetonitrile:water=70:30
Flow rate	: 1.0 mL/min
Column temp.	: 30 $^{\circ}$ C
Pressure	: 4.7 MPa
Detection	: UV 254 nm

### Sample (Order of elution)

1	Uracil
2	Naphthalene

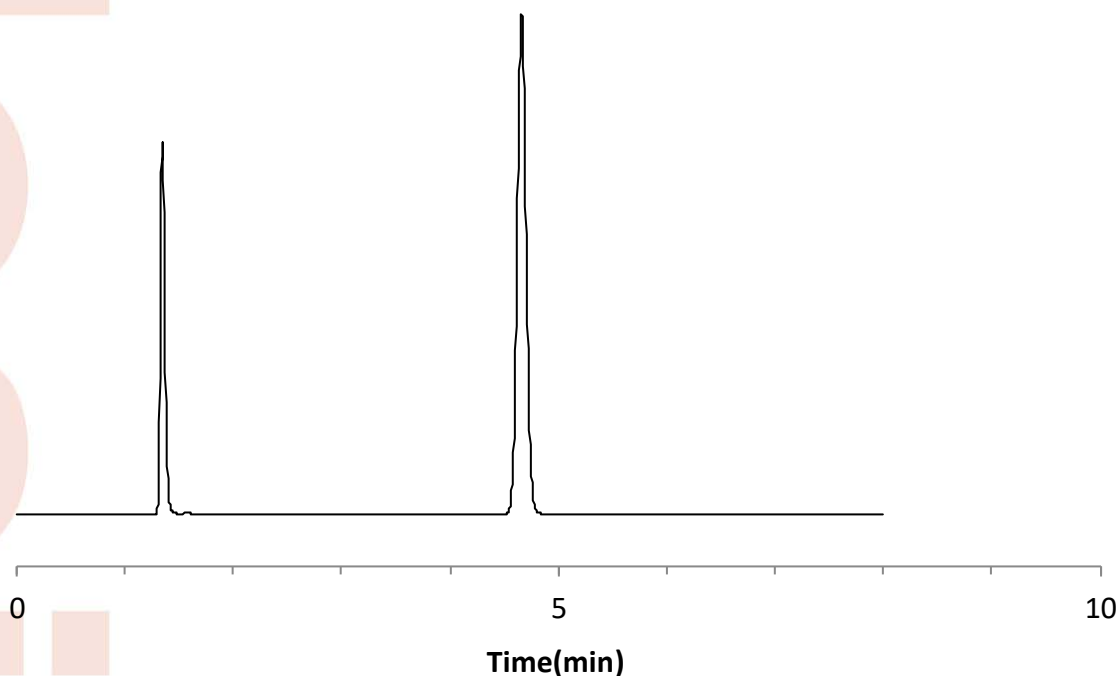

Theoretical plate	(Last peak) $5.54 \times (t_R/W_{0.5})^2 = 15003$
Asymmetry factor	(10% Height of Last peak) = 1.02
Mobile phase at shipment:	Acetonitrile:water=70:30


# Certificate of Analysis

Develosil® ODS-HG, 5µm Batch# 1Y090919

## Analytical Results for Develosil® ODS-HG, 5µm

Analysis of Unbonded Silica Gel		Result
Median Particle Size	[µm]	5.07
Surface Area	[m <sup>2</sup> /g]	296
Pore Volume	[mL/g]	1.06
Average Pore Diameter	[nm]	12.3
Analysis of Bonded Silica Gel		
Total Carbon Content	[%]	19.6

## Chromatographic Results for Develosil® ODS-HG, 5µm

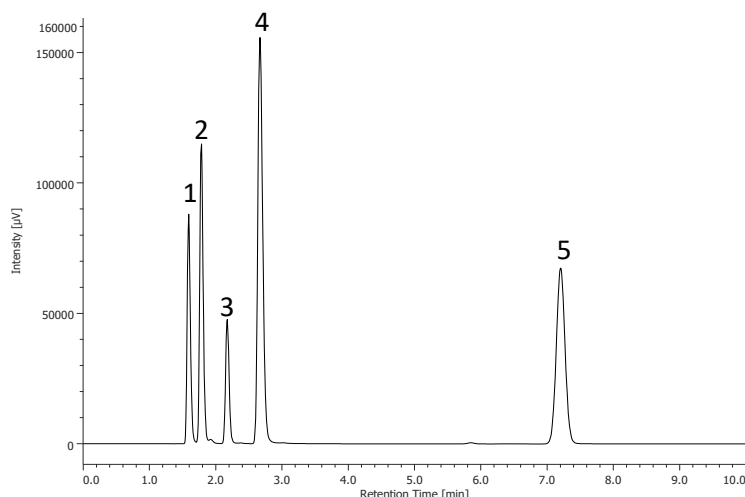

### Sample:

1. Uracil
2. Caffeine
3. Phenol
4. Amitriptyline
5. Naphthalene

### Analytical Conditions;

Column: Develosil ODS-HG, 5µm (4.6x150mm)  
 Mobile phase: Methanol/25mM Ammonium Phosphate, pH3.0=70/30  
 Flow rate: 1.0mL/min  
 Temperature: 40°C  
 Detection: UV254nm  
 Sample: 1.Uracil 2.Caffeine 3.Phenol 4.Amitriptyline 5.Naphthalene  
 Injection volume: 1.0µL

<i>k</i> Naphthalene	Result
	5.61
Relative retention	
<i>k</i> (Caffeine/Naphthalene)	0.03
<i>k</i> (Phenol/Naphthalene)	0.11
<i>k</i> (Amitriptyline/naphthalene)	0.19
<i>k</i> (Caffeine/Phenol)	0.32
Tailing Factor	
Amitriptyline	1.24

 Approved           Ikuo Yamamoto          

 Date:           2019.10.16